

# Ultrasound and CT images

Jason Ali

28/10/2010 10:29:10AM TIS1.1 MI 1.2

Greenhills Ultrasound

C5-1/ABDO

M2



13

FR 28Hz 60°

R1

2D

51%

C 50

P Low

Gen


CE

74%

3000Hz

WF 165Hz

Med

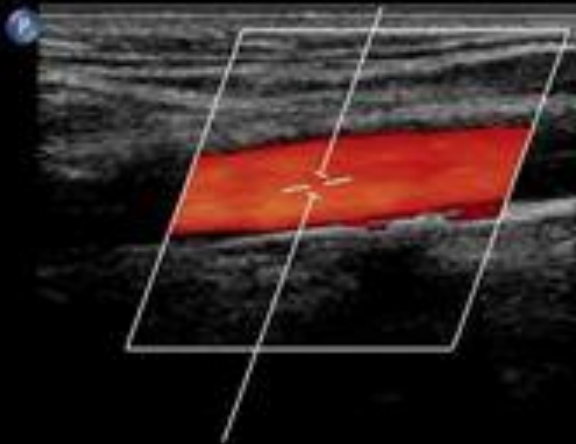

PW

50%

WF 50Hz

SV 1.5mm


M2

3.5MHz


1.3cm


M2 M3

+28.9

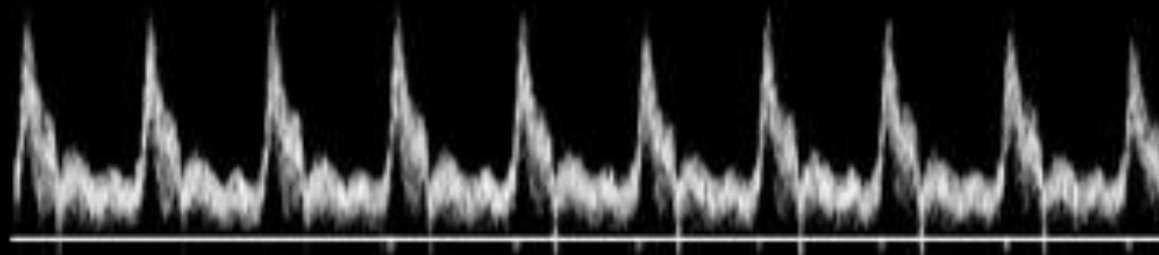

6.5sec

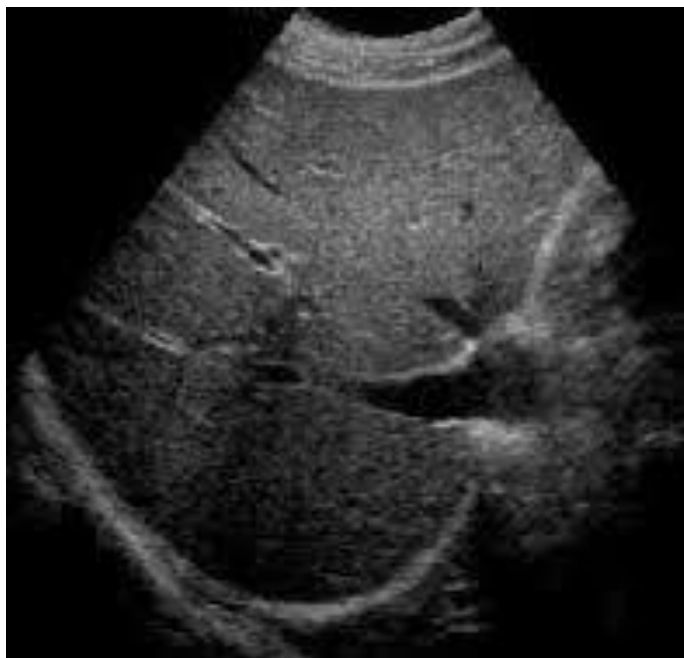

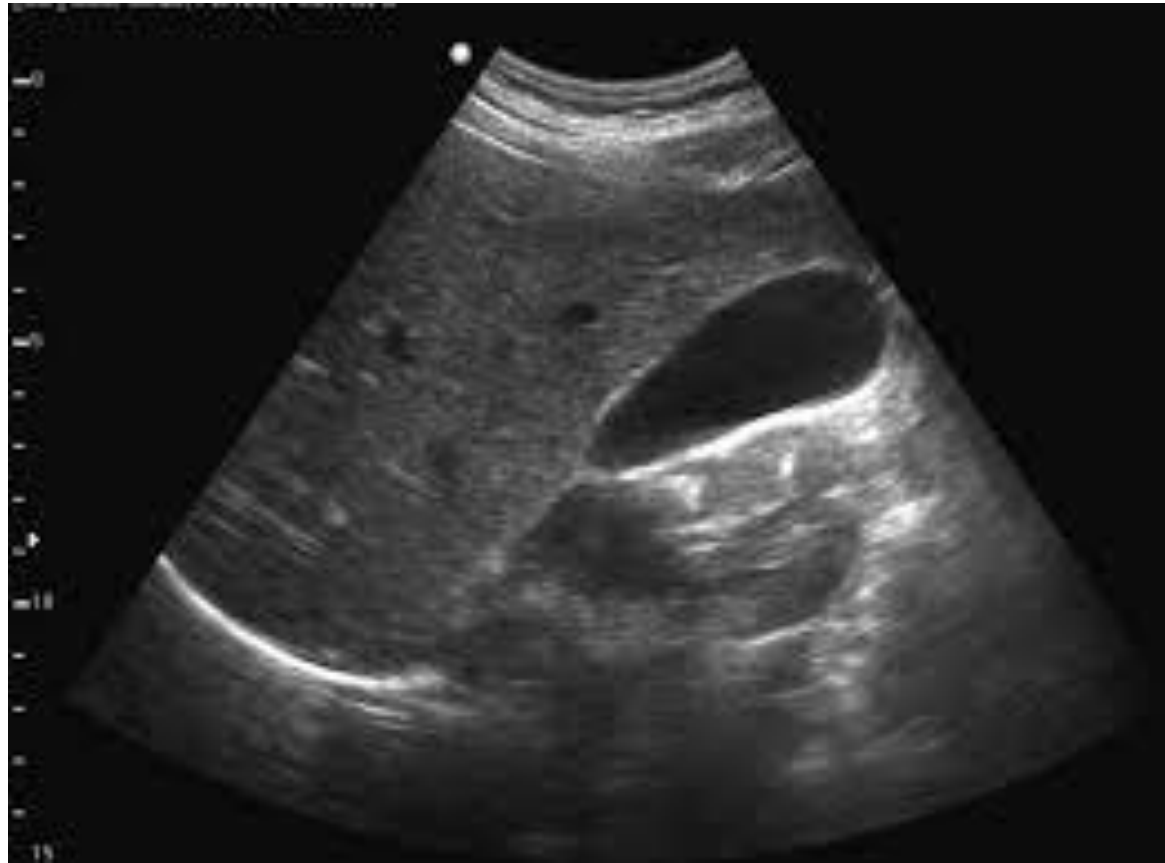












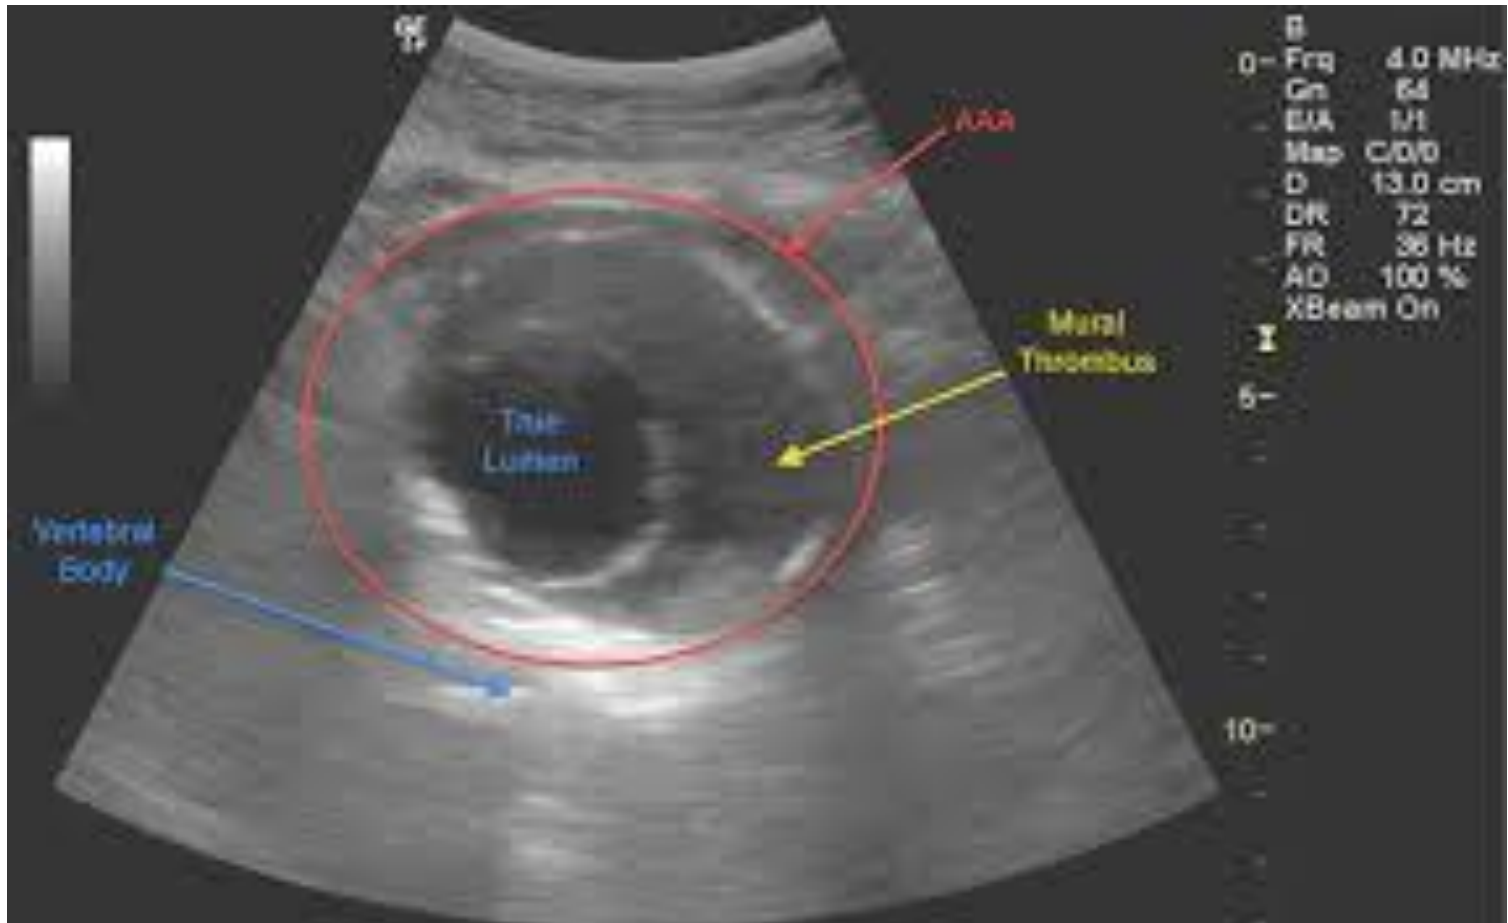



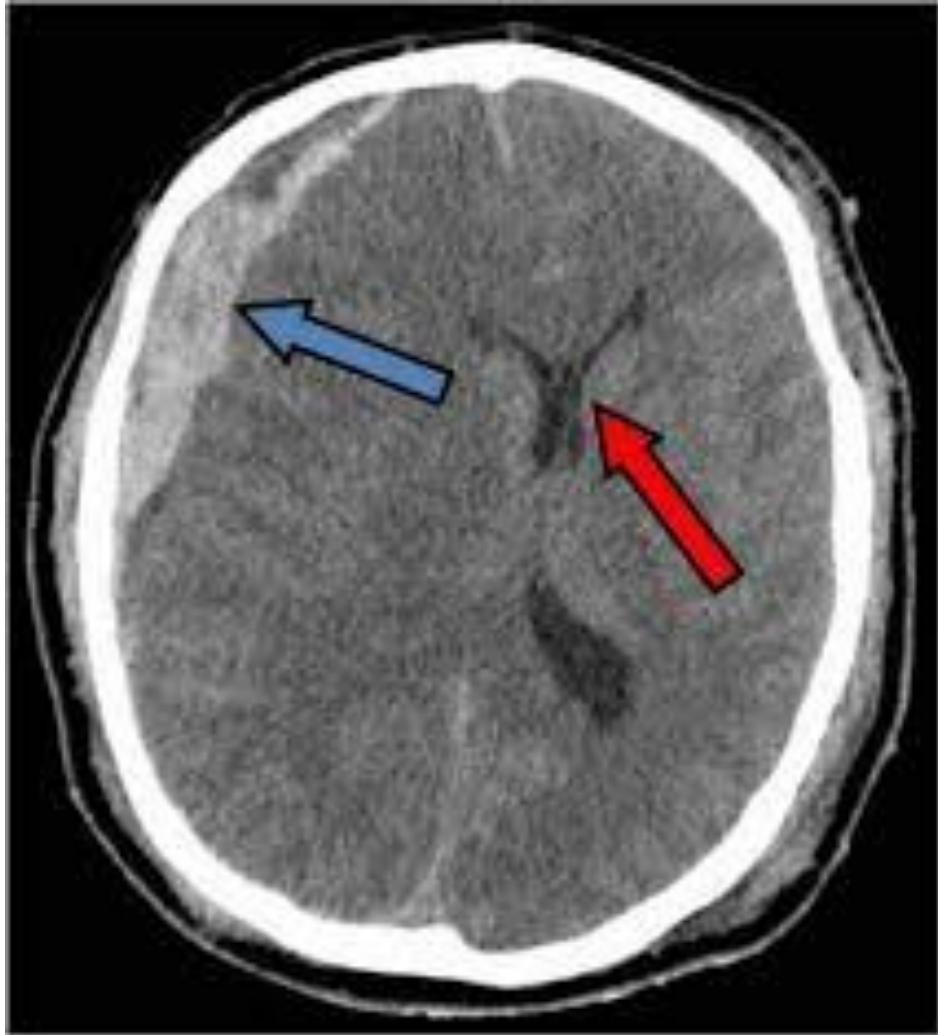

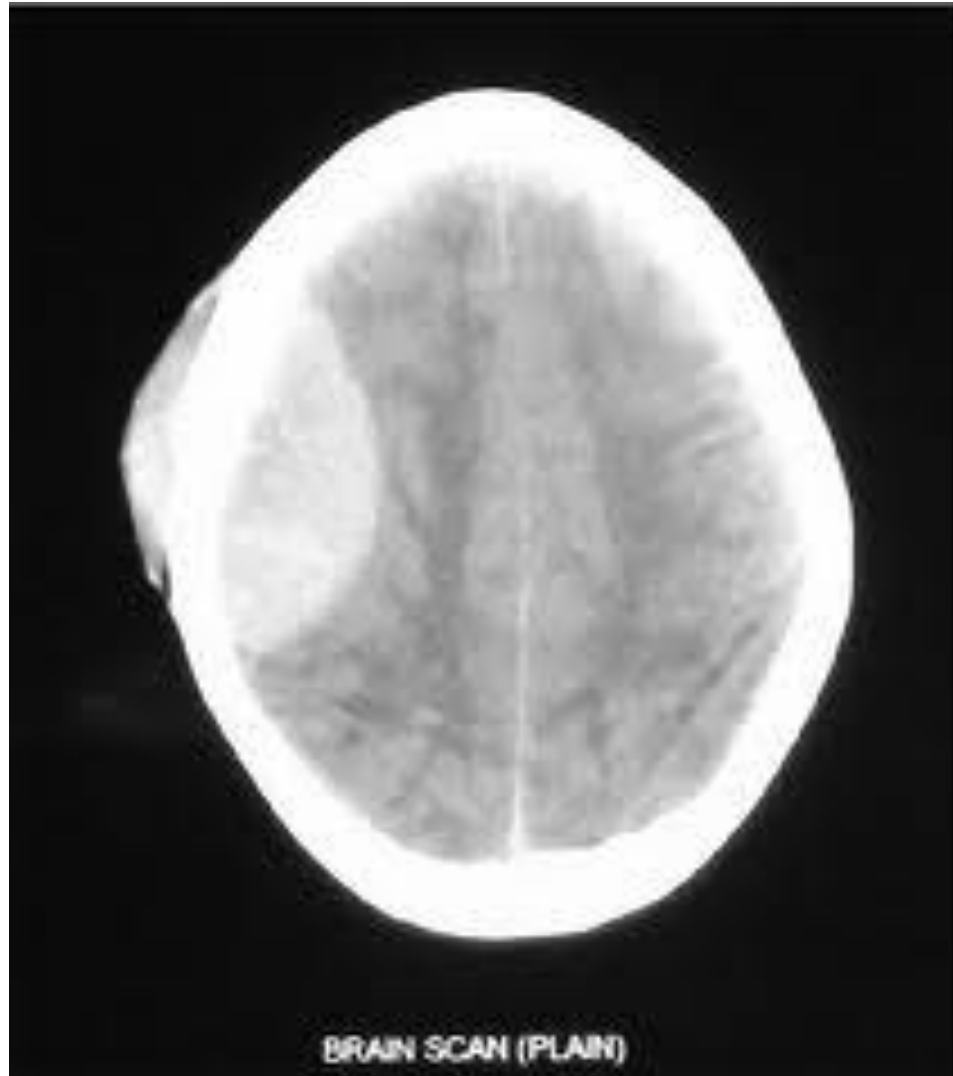

Brilliance16  
Ex: 83908

A<sub>0</sub>

Credit Valley

C: CONTRAST  
Ser: 315  
Im: 27/56  
Ax: H579.0 (COI)

Acc: 003296920  
2012 Aug 01  
Acq Tm: 14:56:38

512 x 512  
LB

R

L

120.0 kV  
200.0 mA  
3.0 mm/0.0:1Tilt: -15.0  
1.8 s  
Lin:DCM / Lin:DCM / 1640  
W:80 L:40

DFOV: 23.4 x 23.4cm



1000  
0.00


Department of Radiology  
General Hospital




1000  
0.00  
1000  
0.00

1000  
0.00



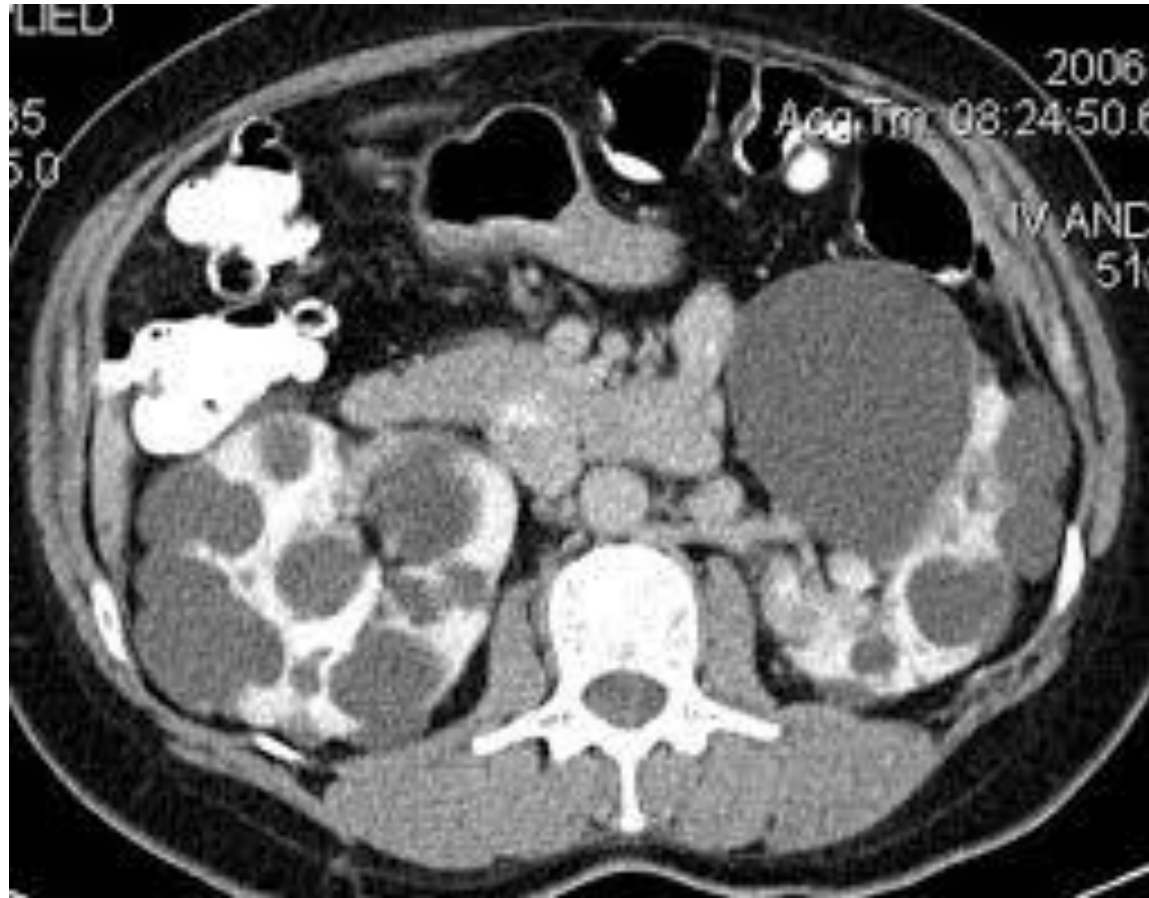



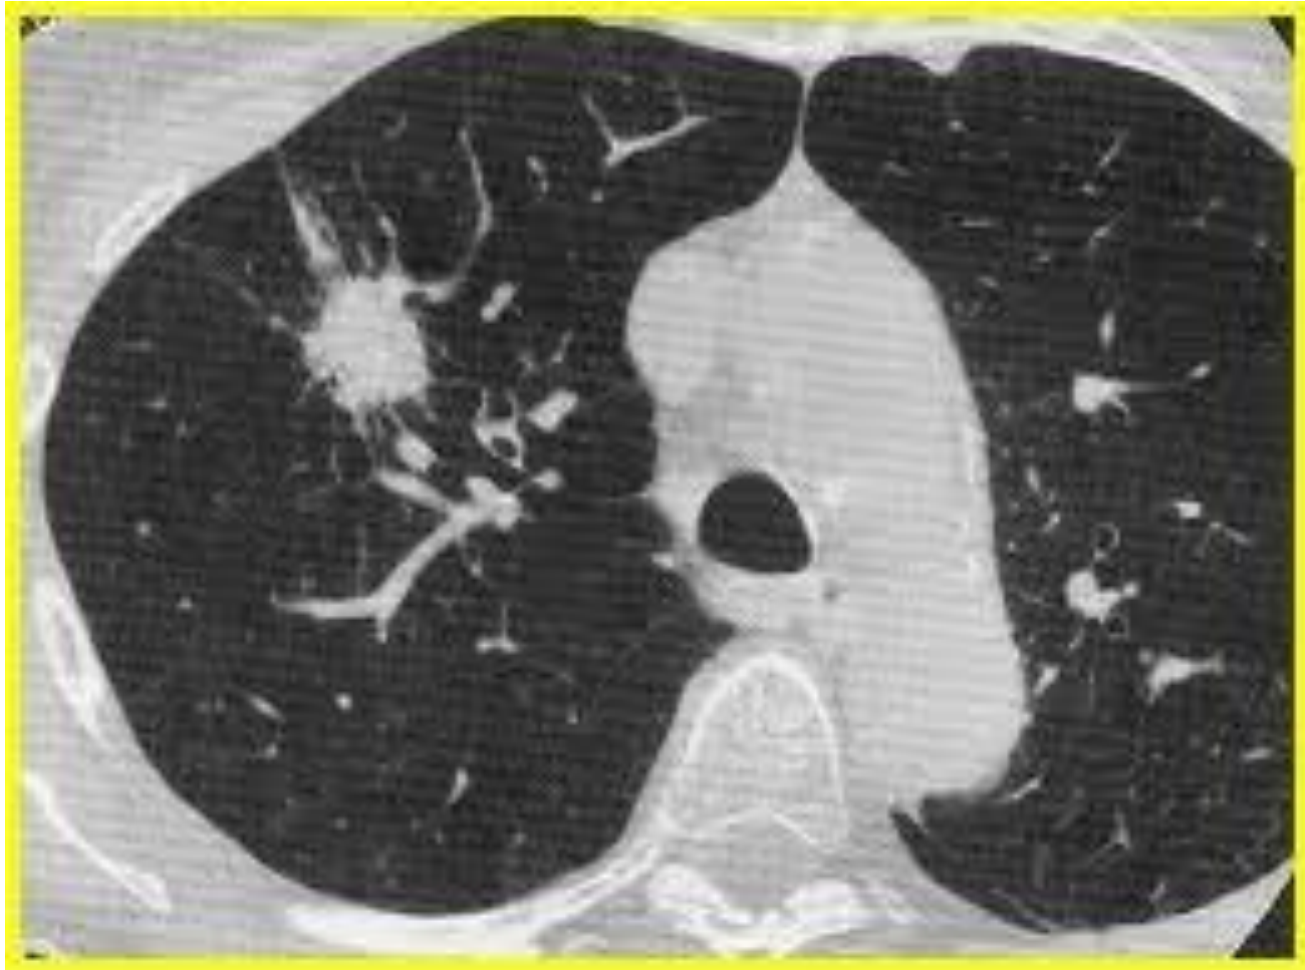



56

[A]

XRAY-CT ABD W/CON

6/7/2008

3:19:24 PM



SP: 284.5 mm

ST: 5.0 mm

C40

W400

Not for diagnostic use